



Shoulder Stabilizer Instructions

⚠ WARNINGS ⚠

CAUTION: FEDERAL LAW RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A LICENSED HEALTH CARE PRACTITIONER.






CAUTION: FOR SINGLE PATIENT USE ONLY.

CAUTION: IF YOU EXPERIENCE INCREASED PAIN, SWELLING, OR ANY ADVERSE REACTIONS WHILE USING THIS PRODUCT, IMMEDIATELY CONSULT YOUR MEDICAL PROFESSIONAL.

CAUTION: IF AN ALLERGY TO NEOPRENE EXISTS OR A RASH DEVELOPS DISCONTINUE USE IMMEDIATELY.

WARNING: CAREFULLY READ USE INSTRUCTIONS AND WARNINGS PRIOR TO OPERATION.

WARNING: THIS DEVICE WILL NOT PREVENT OR REDUCE ALL INJURIES. PROPER REHABILITATION AND ACTIVITY MODIFICATION ARE ALSO AN ESSENTIAL PART OF A SAFE TREATMENT PROGRAM.

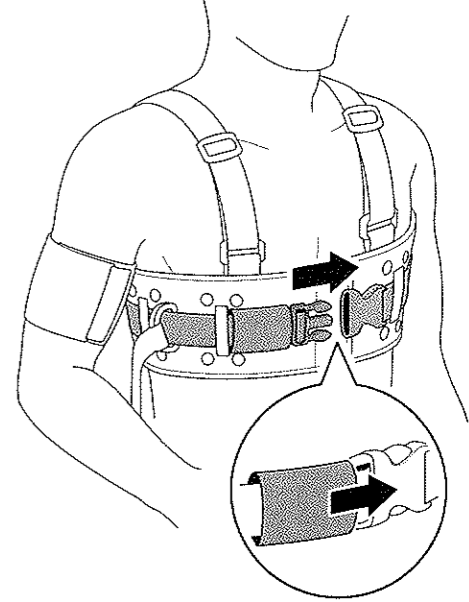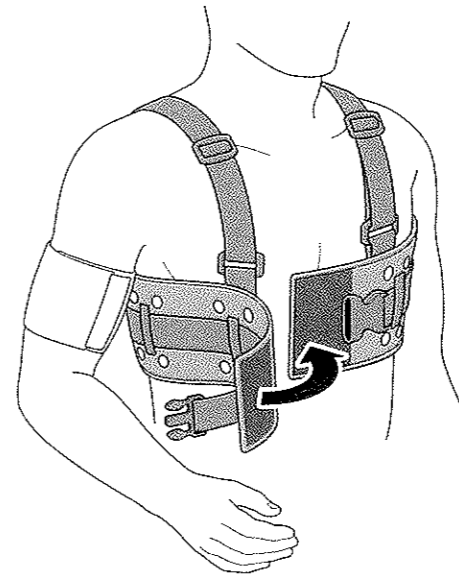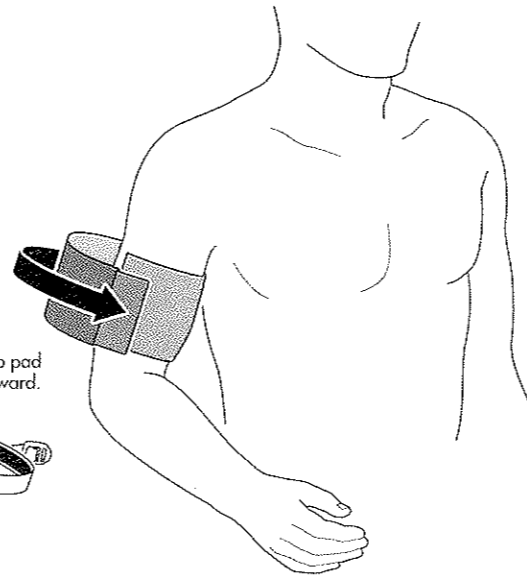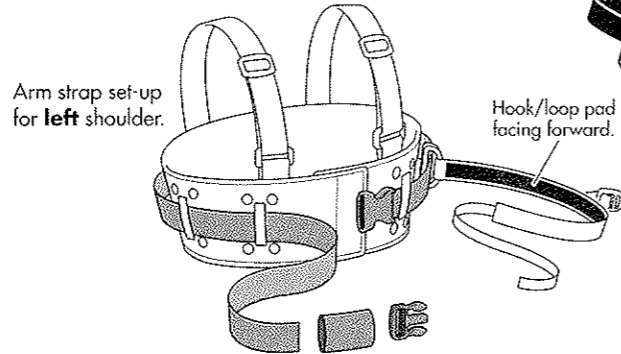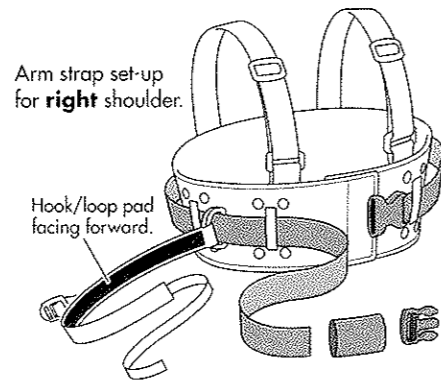


1 Brace can be used for left or right shoulder. To change sides, remove buckle on chest strap, slide off arm strap and apply to opposite side. Be sure that hook/loop pad is facing forward.

2 Secure neoprene arm wrap to bicep on affected arm/shoulder. Wrap should be applied directly to skin to prevent migration.


3 Apply chest harness. Adjust buckles and suspenders to desired tension. Slide neoprene buckle cover into place.

Sizing	Chest circumference (at level of axilla)
Small	34" – 38"
Medium	38" – 42"
Large	42" – 46"
X Large	46" – 51"
XX Large	51" – 56"


HAND WASH/DRIP DRY

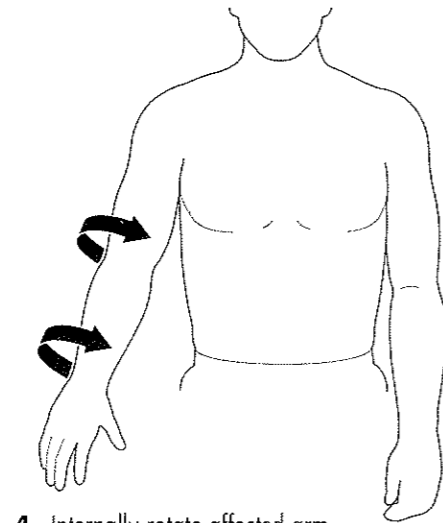


4 Internally rotate affected arm.

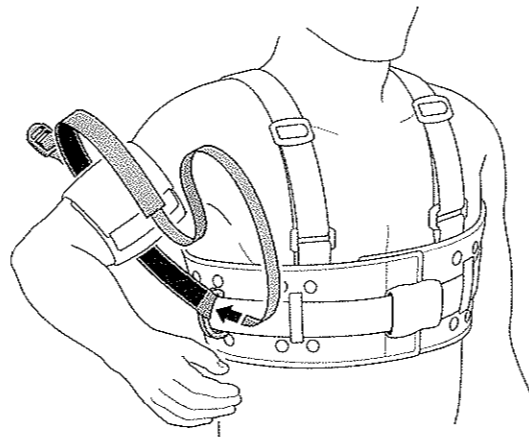

5 Position arm for desired restriction. Apply arm strap over arm wrap from back side. Feed strap end through chest belt D-rings.

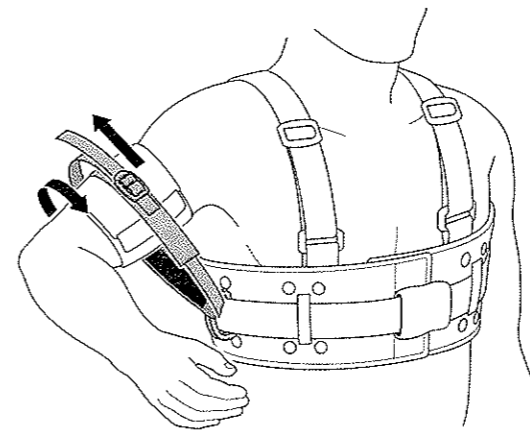

6 Feed arm strap end through buckle to form a continuous loop, tighten to desired level of arm movement restriction.

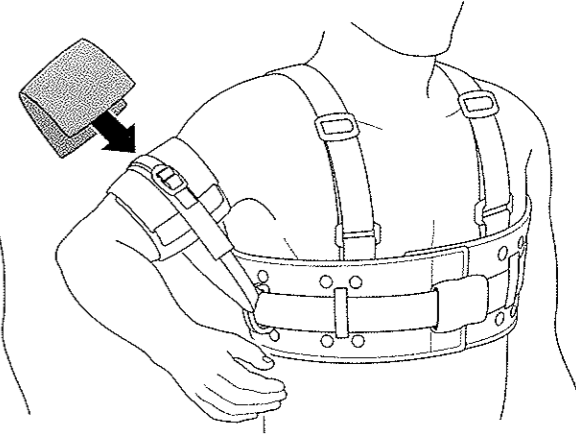

7 Cover arm assembly with elastic wrap to cover plastic buckle and secure loose strap ends.

Excess straps may be cut to desired length. Melt ends to prevent fraying.